
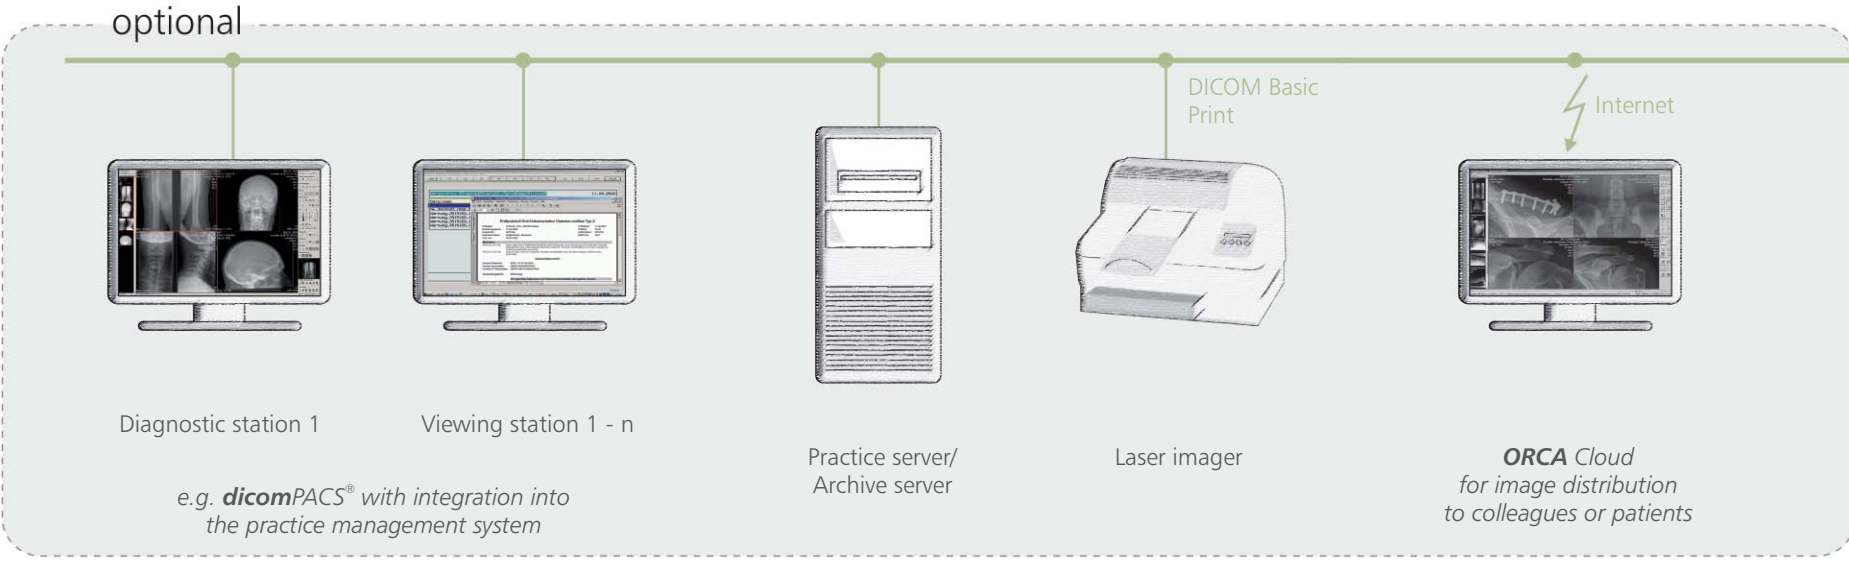


1. Upgrade existing **stationary** X-ray systems

Mode of operation: **one** wireless X-ray detector for all systems

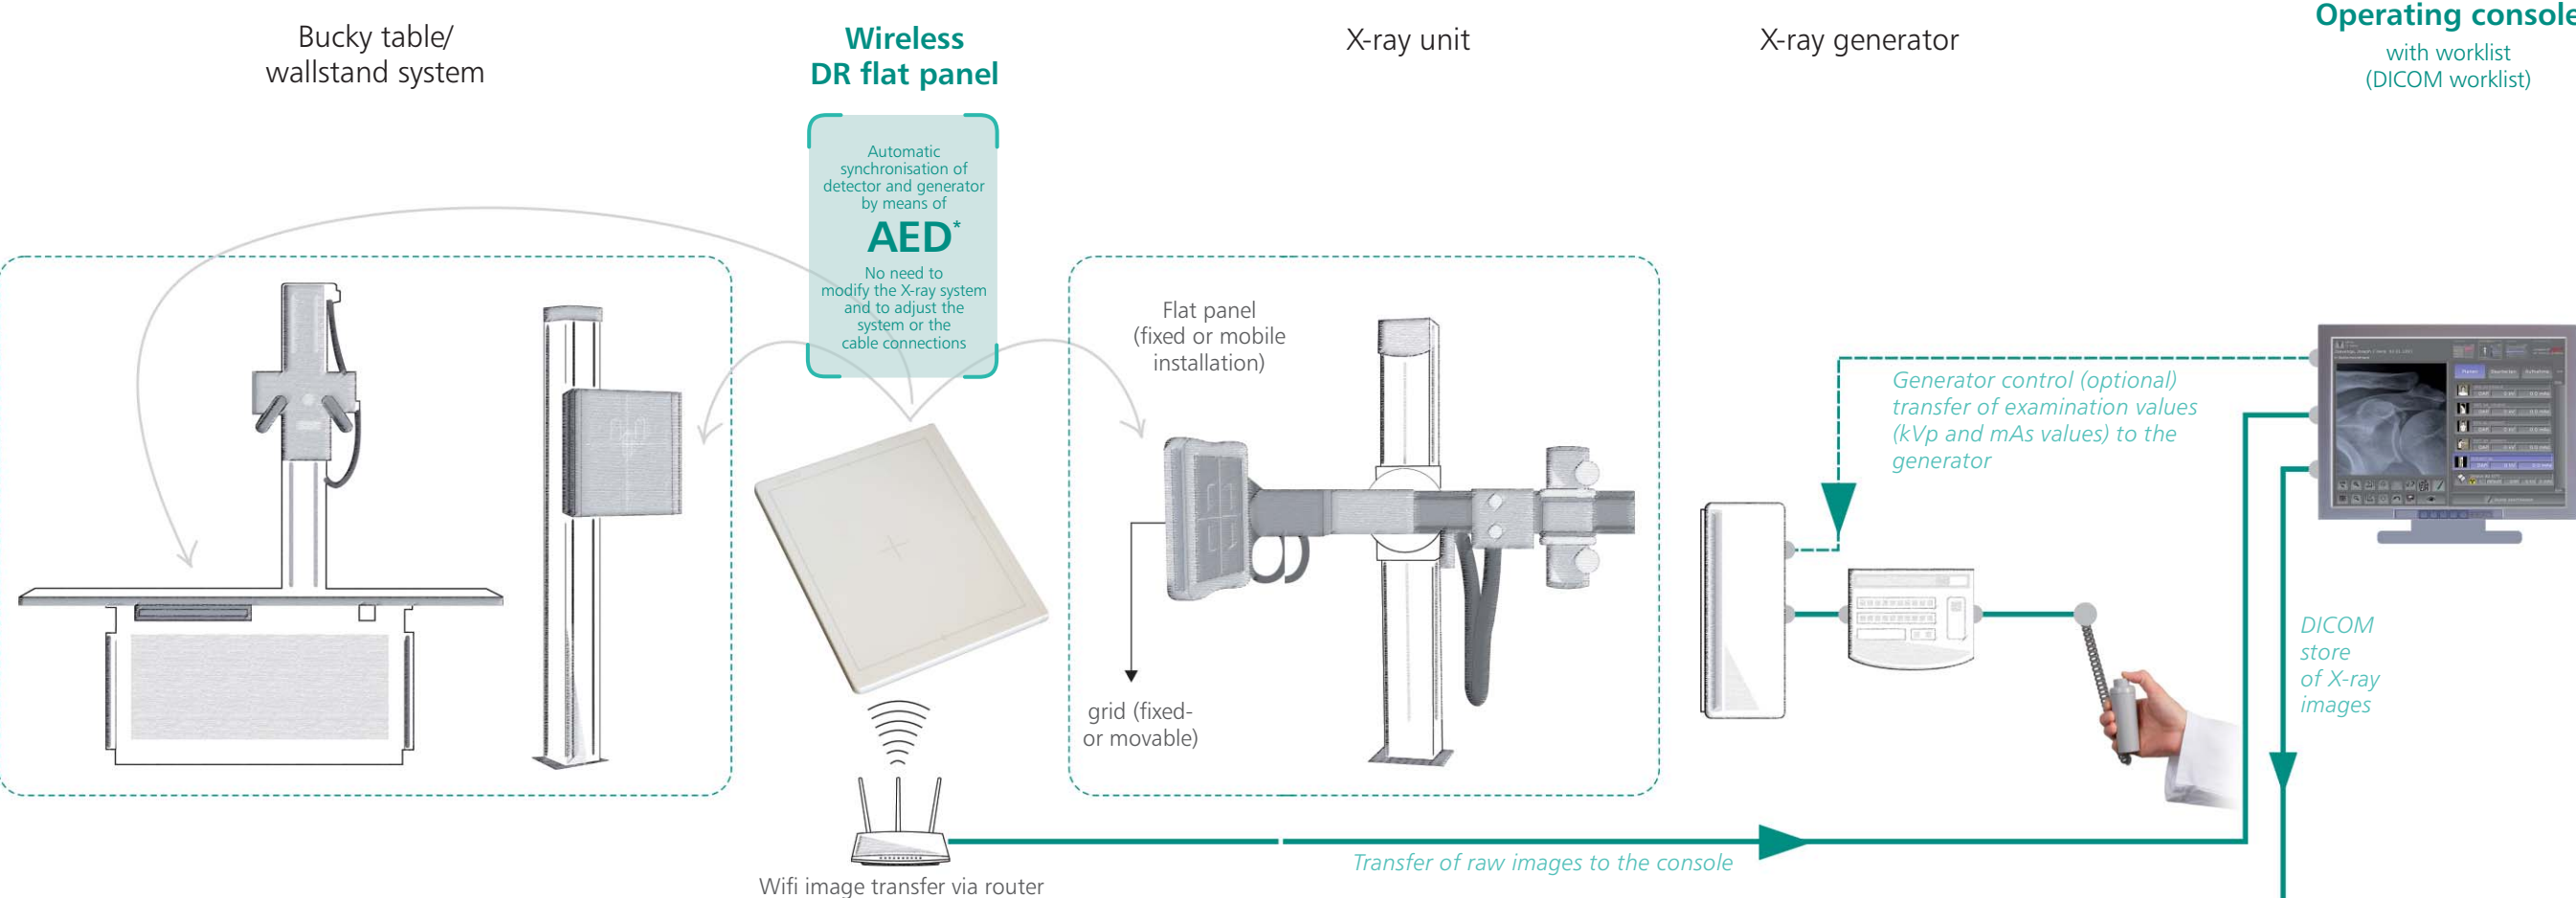

**Medici DR Systems**

\* Auto Exposure Detection